


The 510k process which SHOULD have happened with the DePuy ASR Modular Acetabular Cup System



The 510k process that DID happen with the DePuy ASR Modular Acetabular Cup System

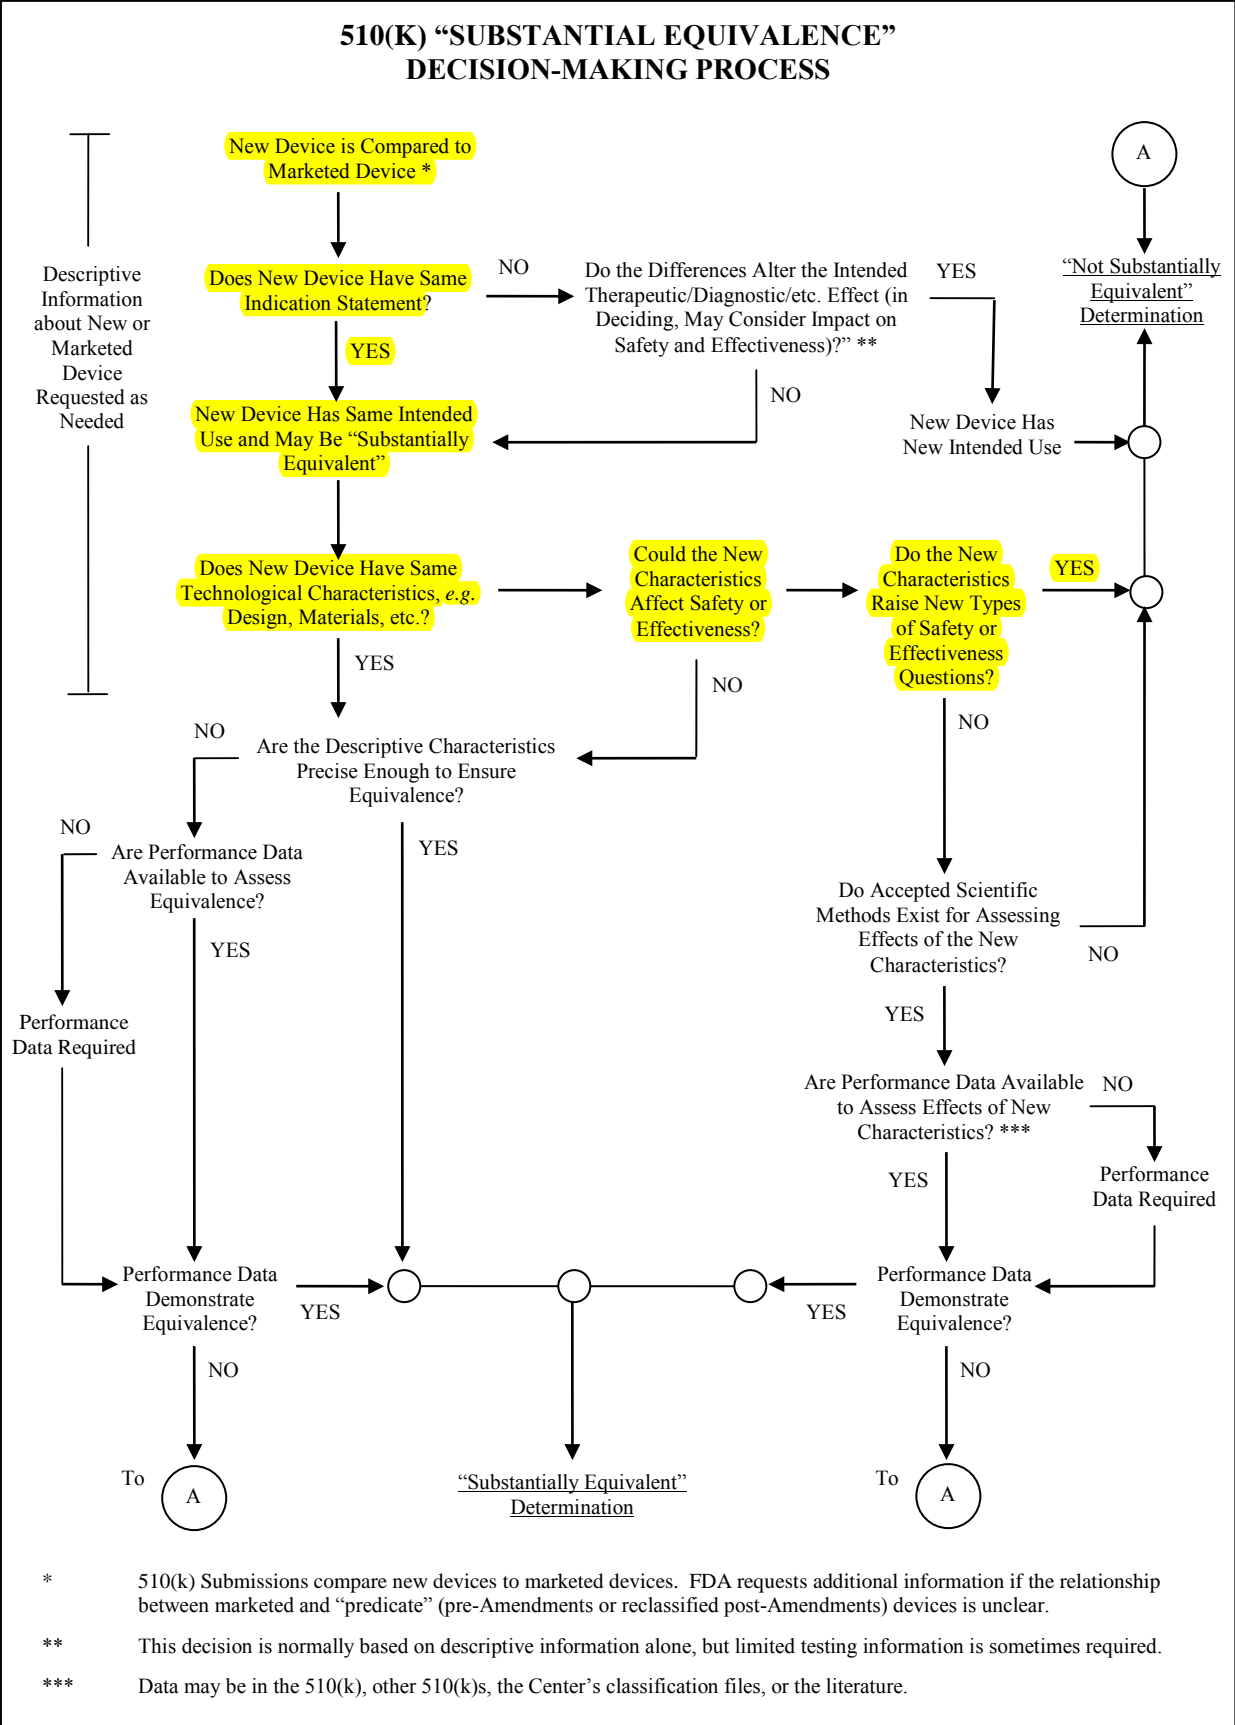